

Title: METHOD AND SYSTEM FOR PRESENTING DIGITAL MEDIA

Inventors: Tom C. Hill and Robin L. Thompson

Docket No.: QBEO117566

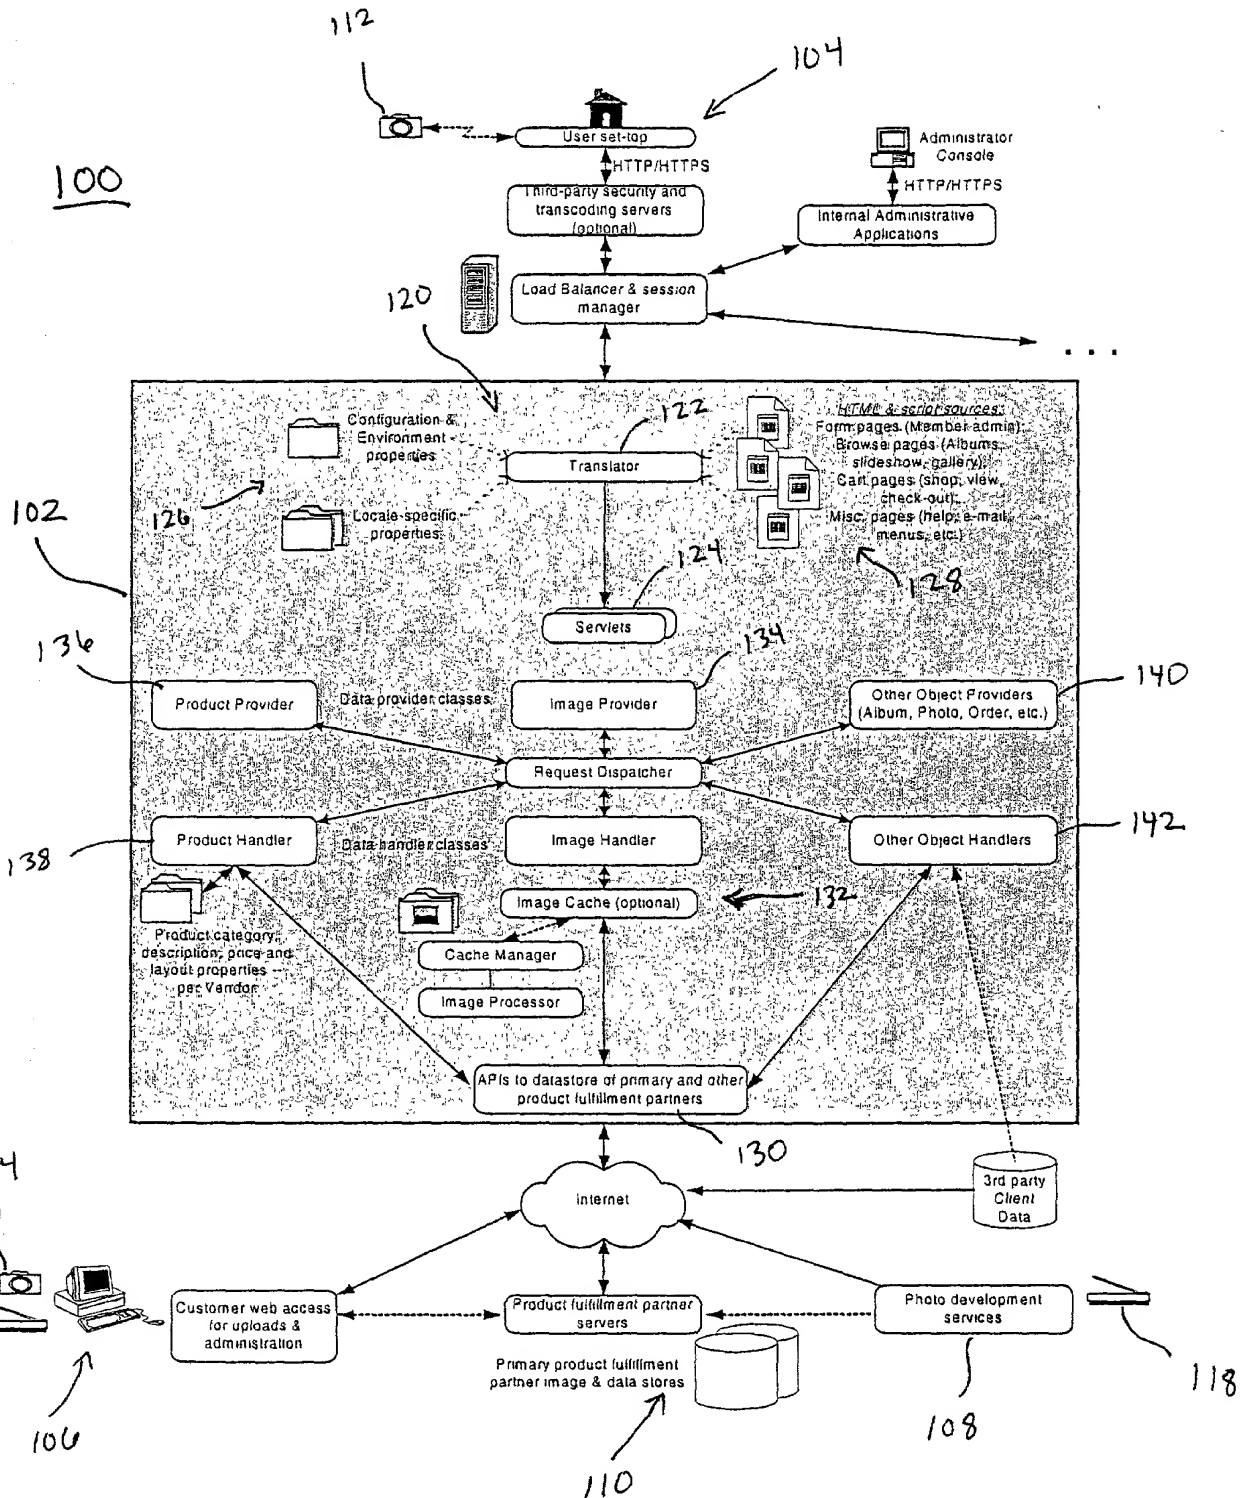


Fig. 1

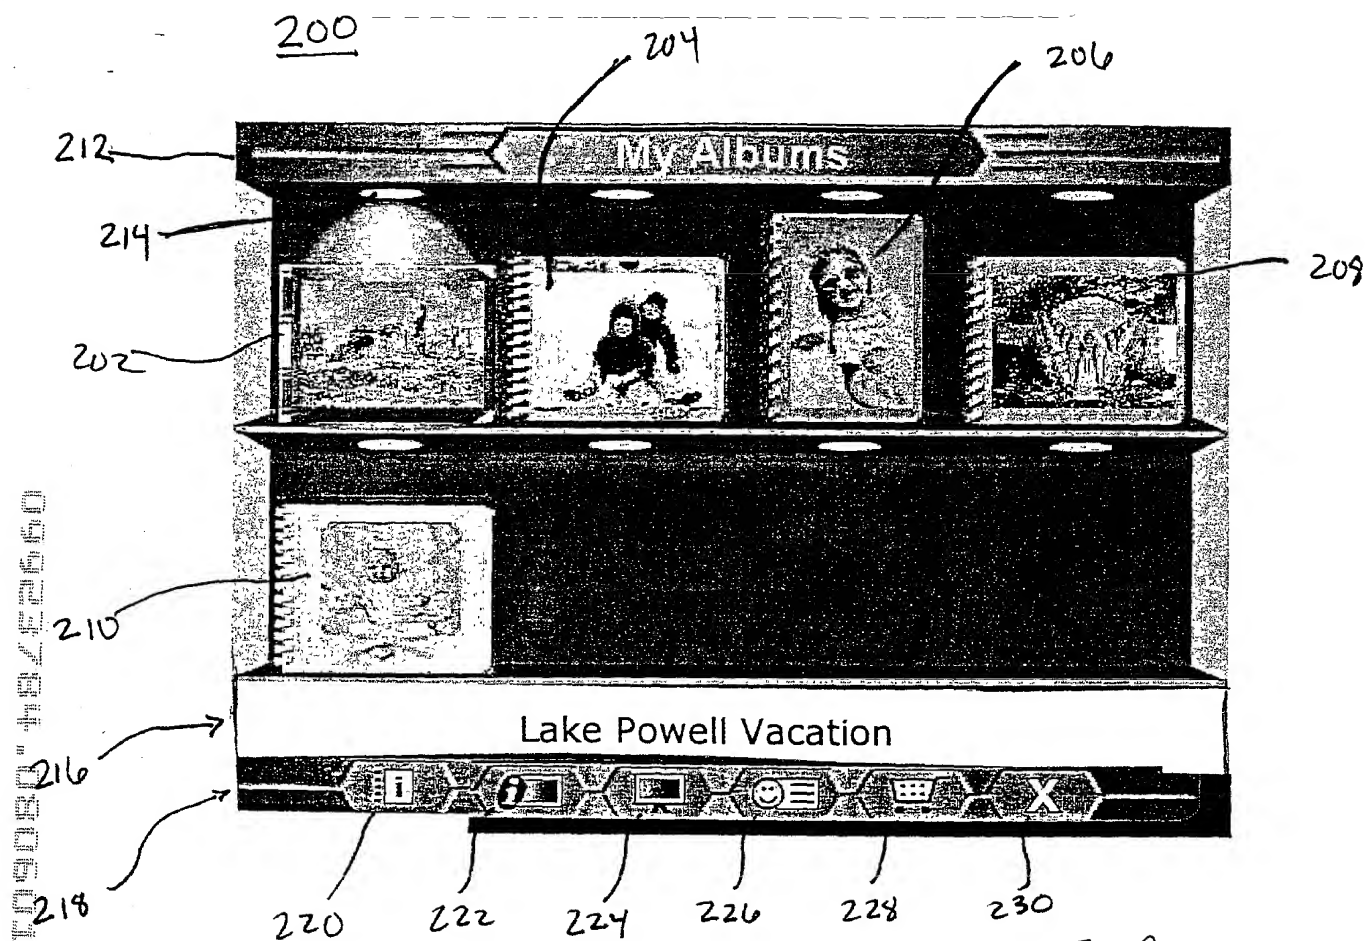


Fig. 2







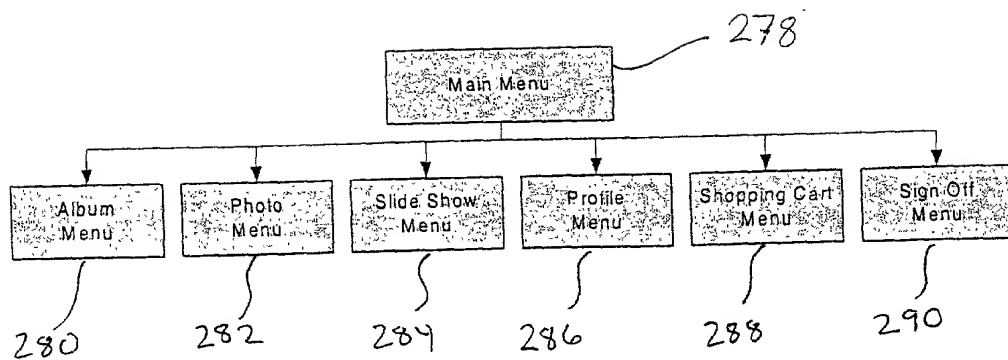


Fig. 7

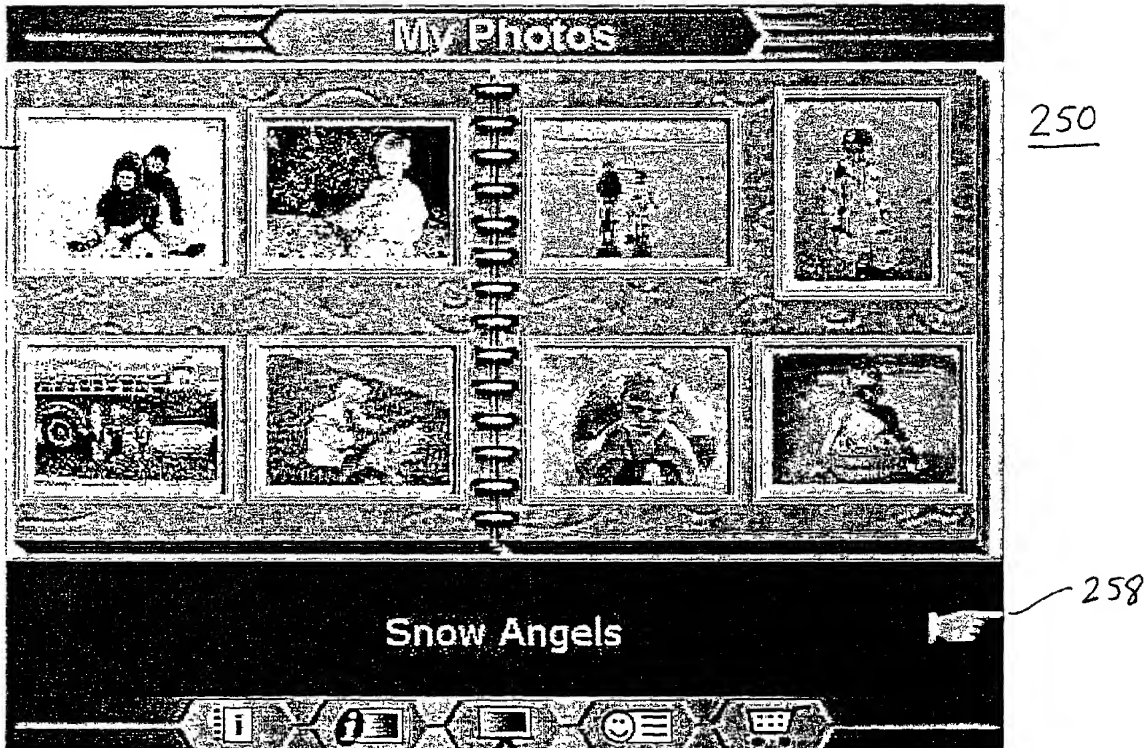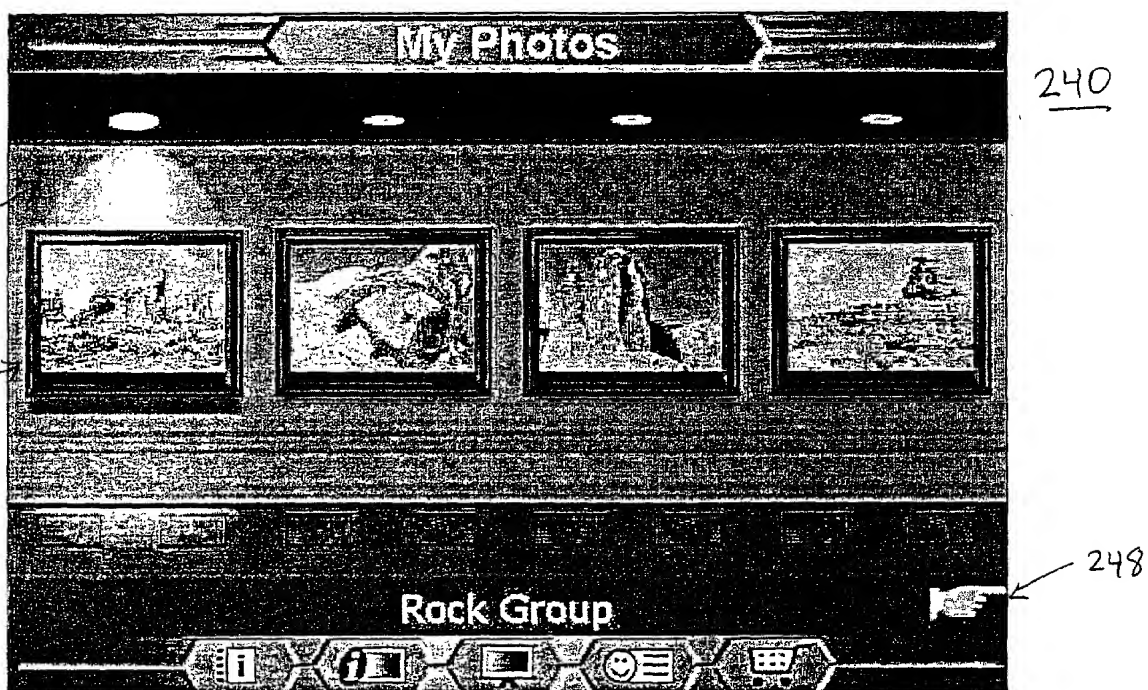

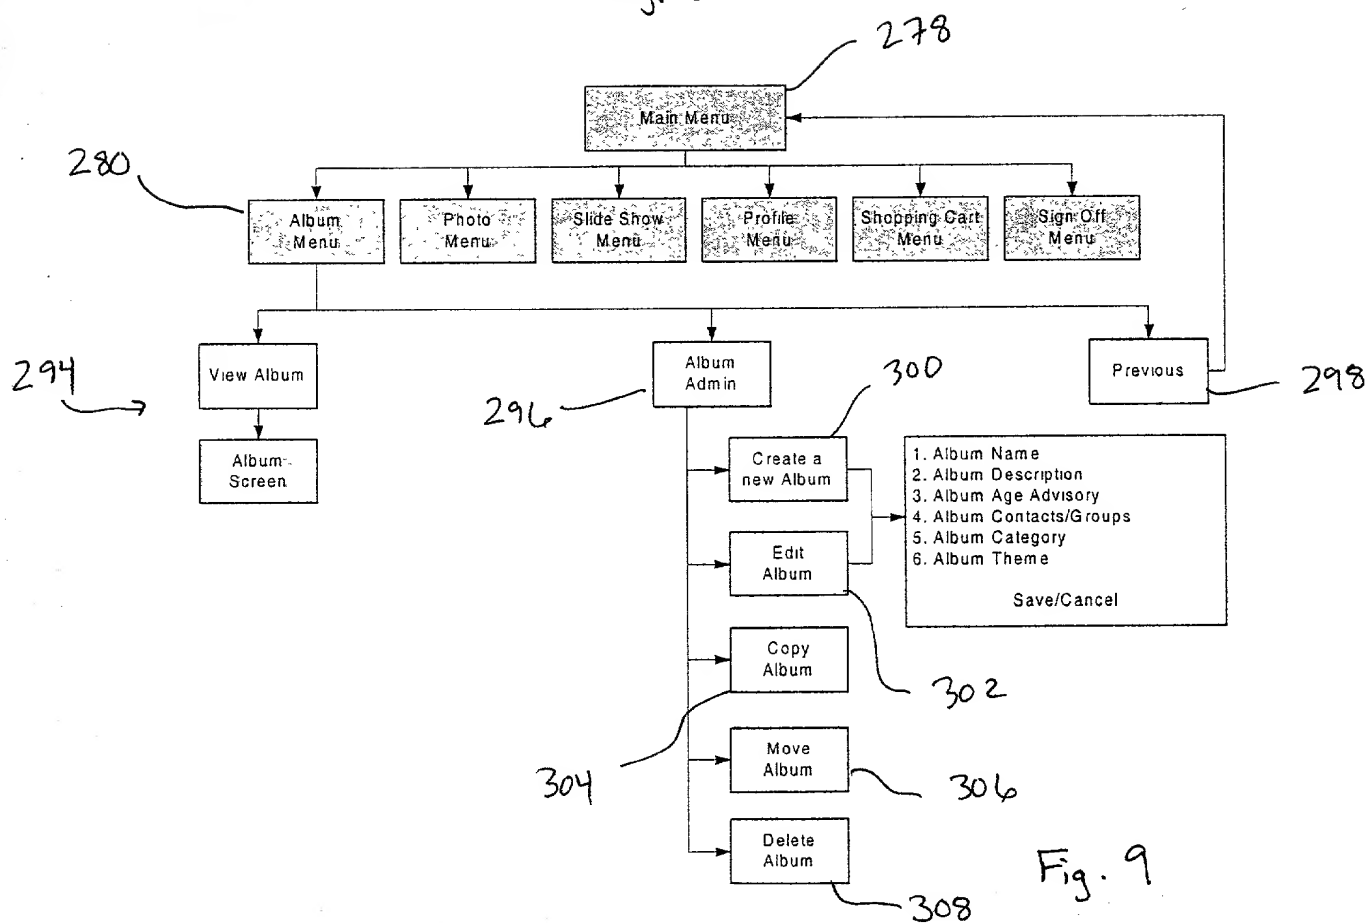

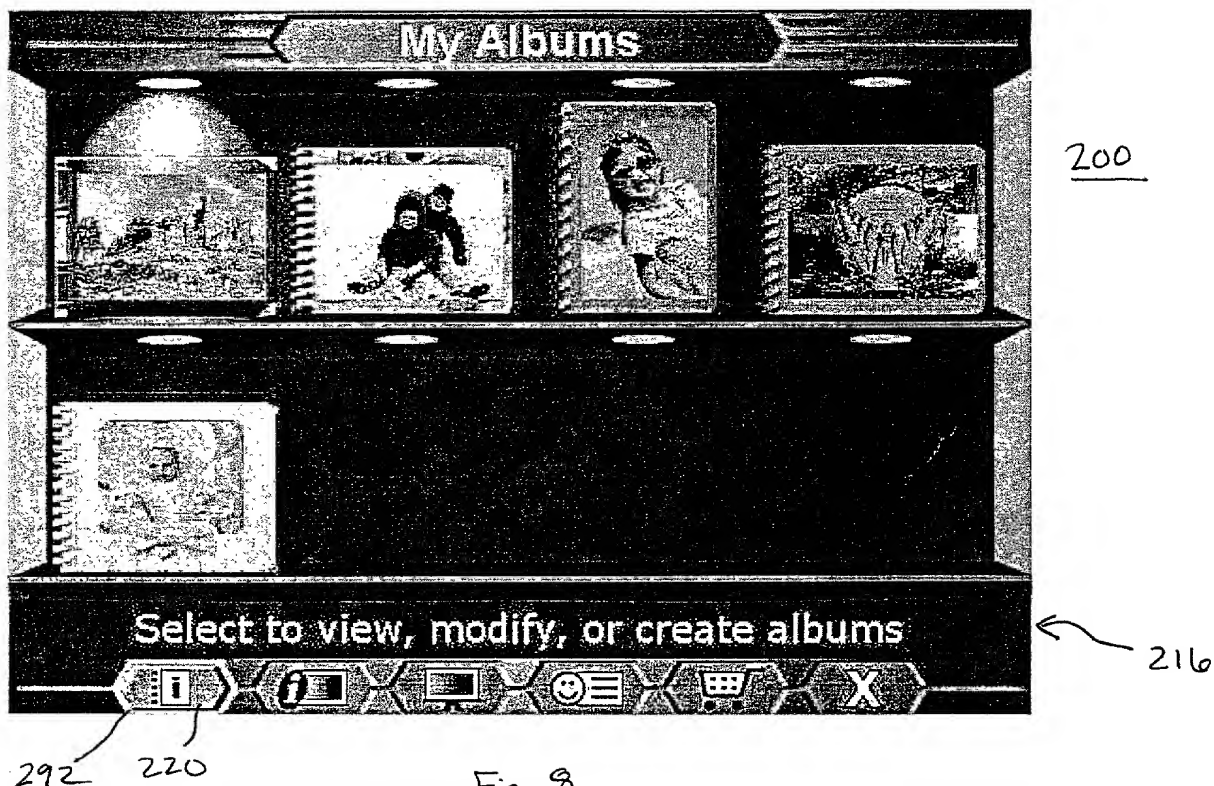

Title: METHOD AND SYSTEM FOR PRESENTING DIGITAL MEDIA

Inventors: Tom C. Hill and Robin L. Thompson

Docket No.: QBEO117566

284

278

310

312

314

316

318

320

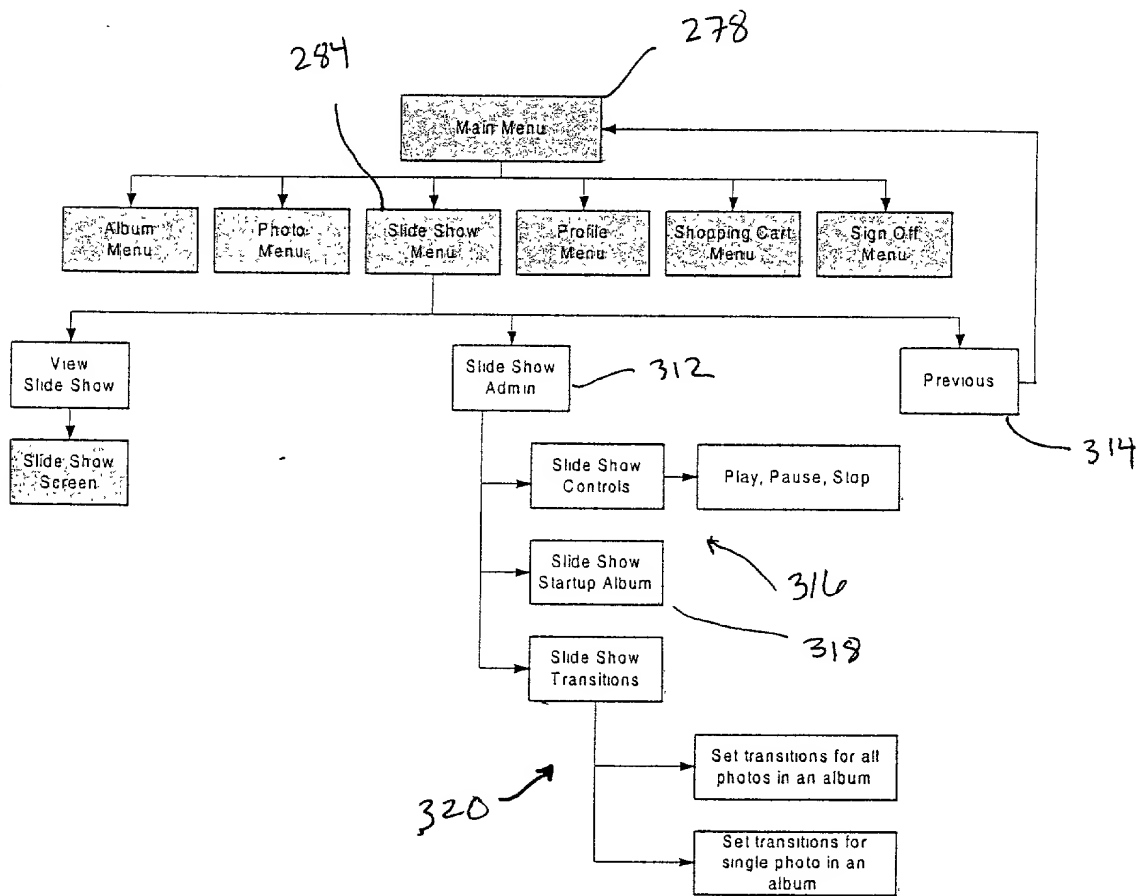


Fig. 10

Title: METHOD AND SYSTEM FOR PRESENTING DIGITAL  
MEDIA

Inventors: Tom C. Hill and Robin L. Thompson

Docket No.: QBEO117566

330


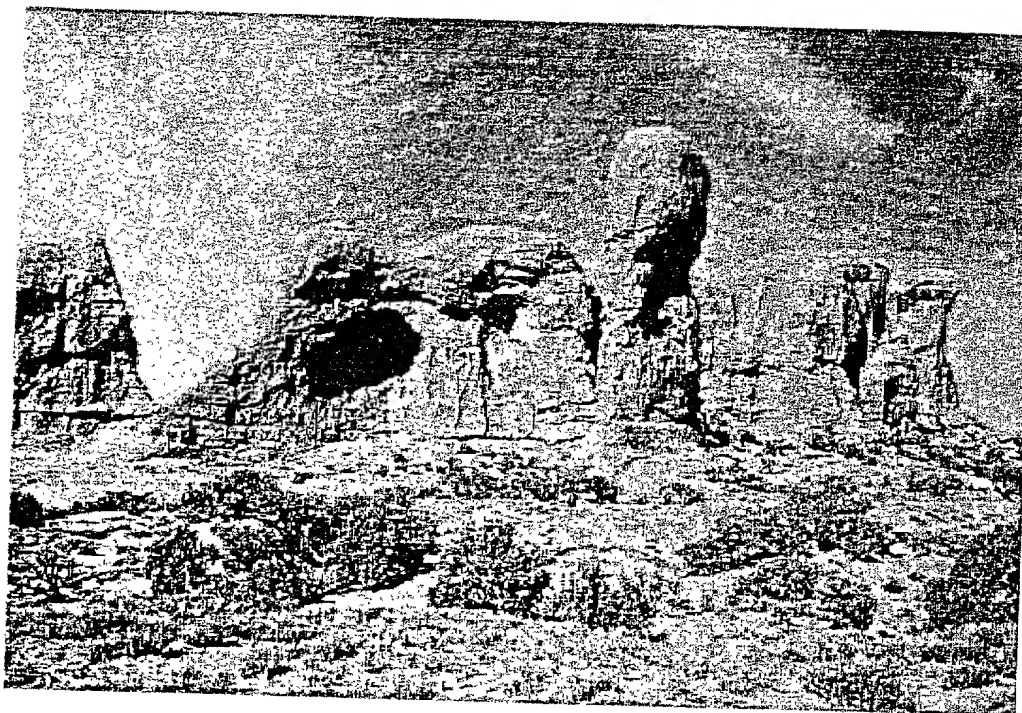


Fig. 11

340

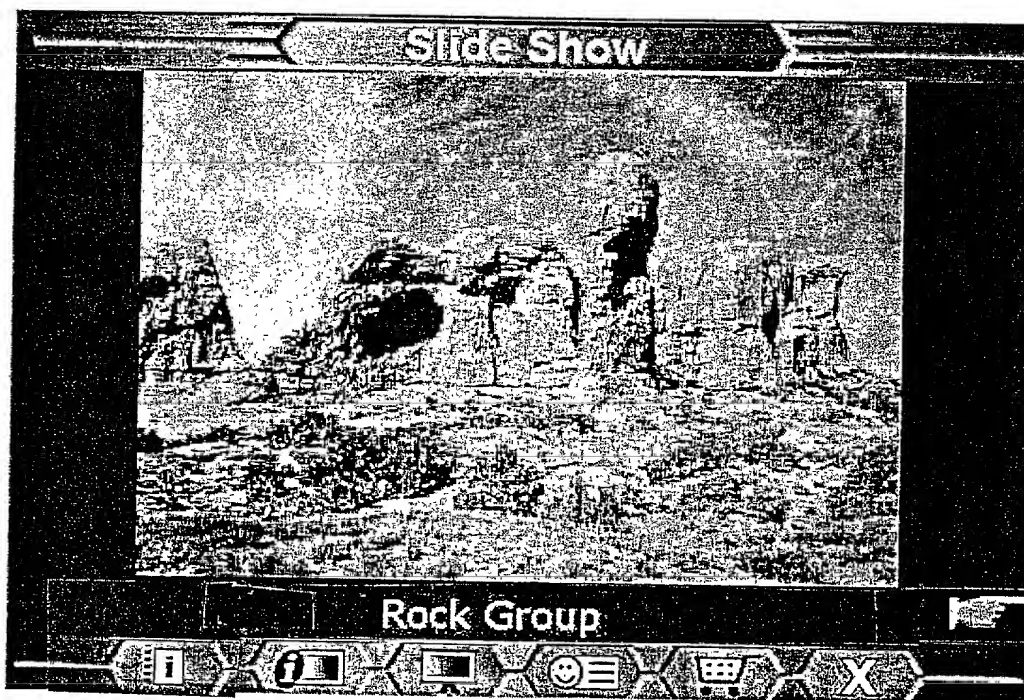

342 →

→ 344

218 ↗

Fig. 12

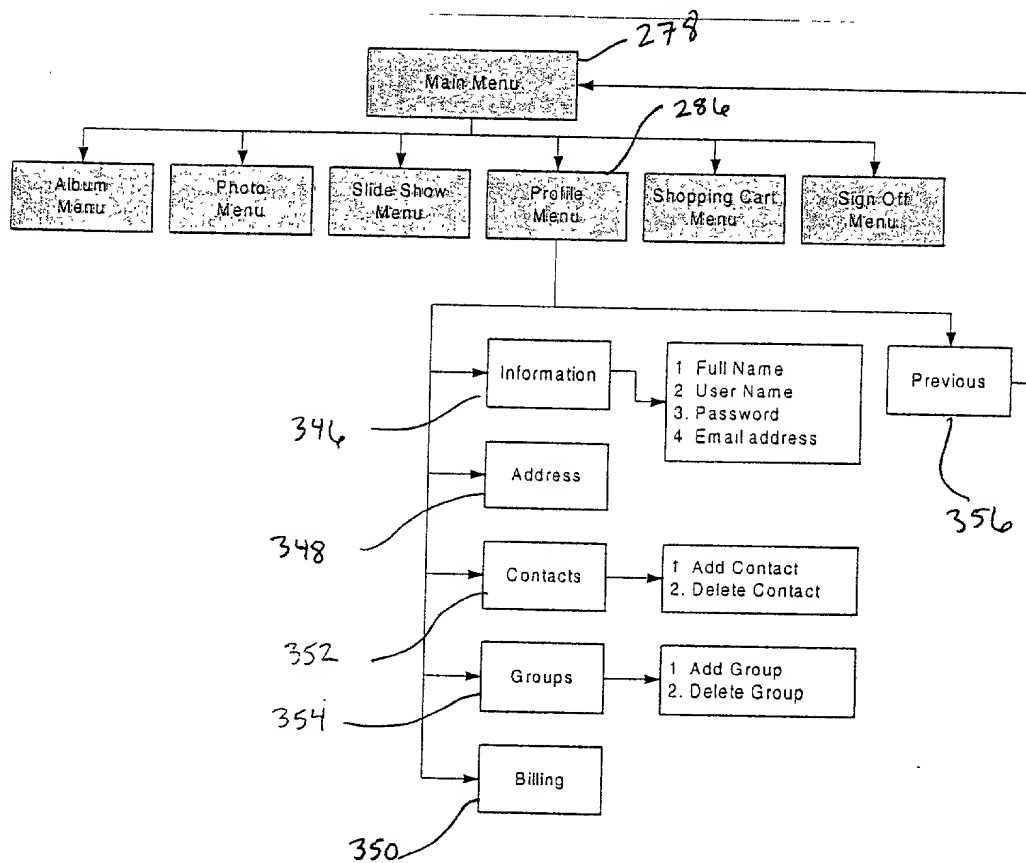


Fig. 13







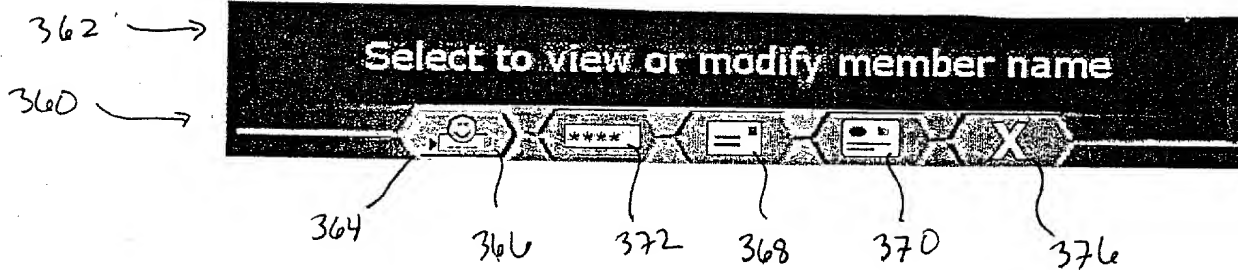


Fig. 14

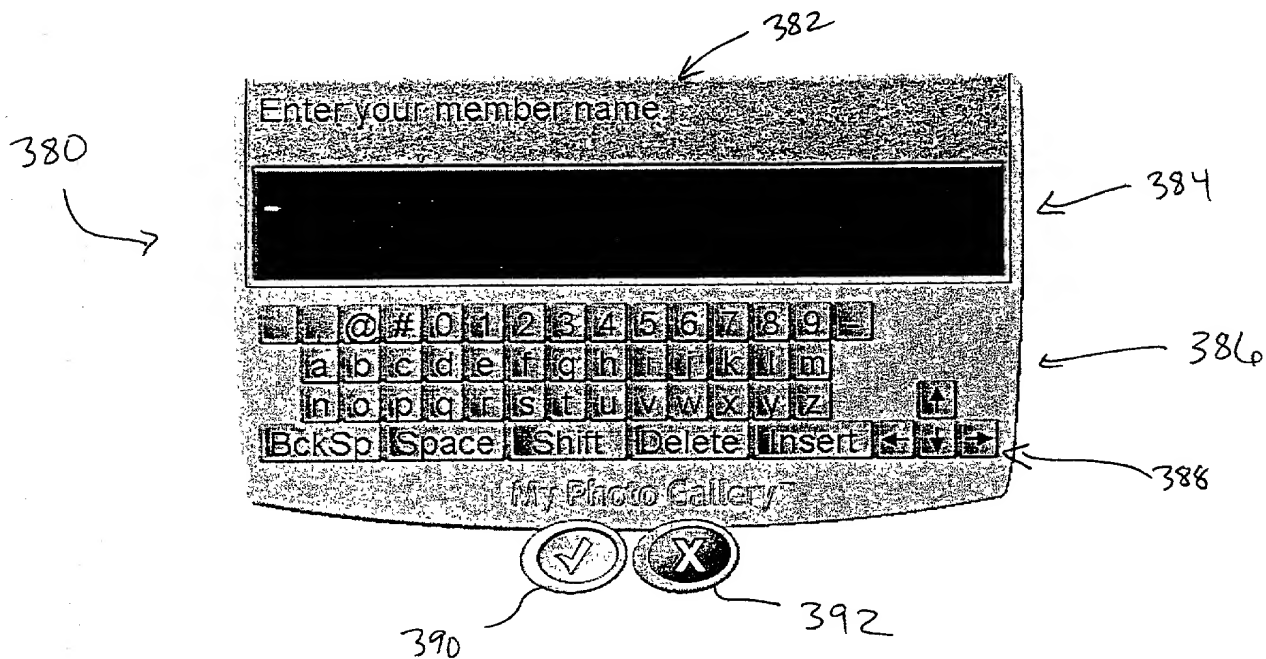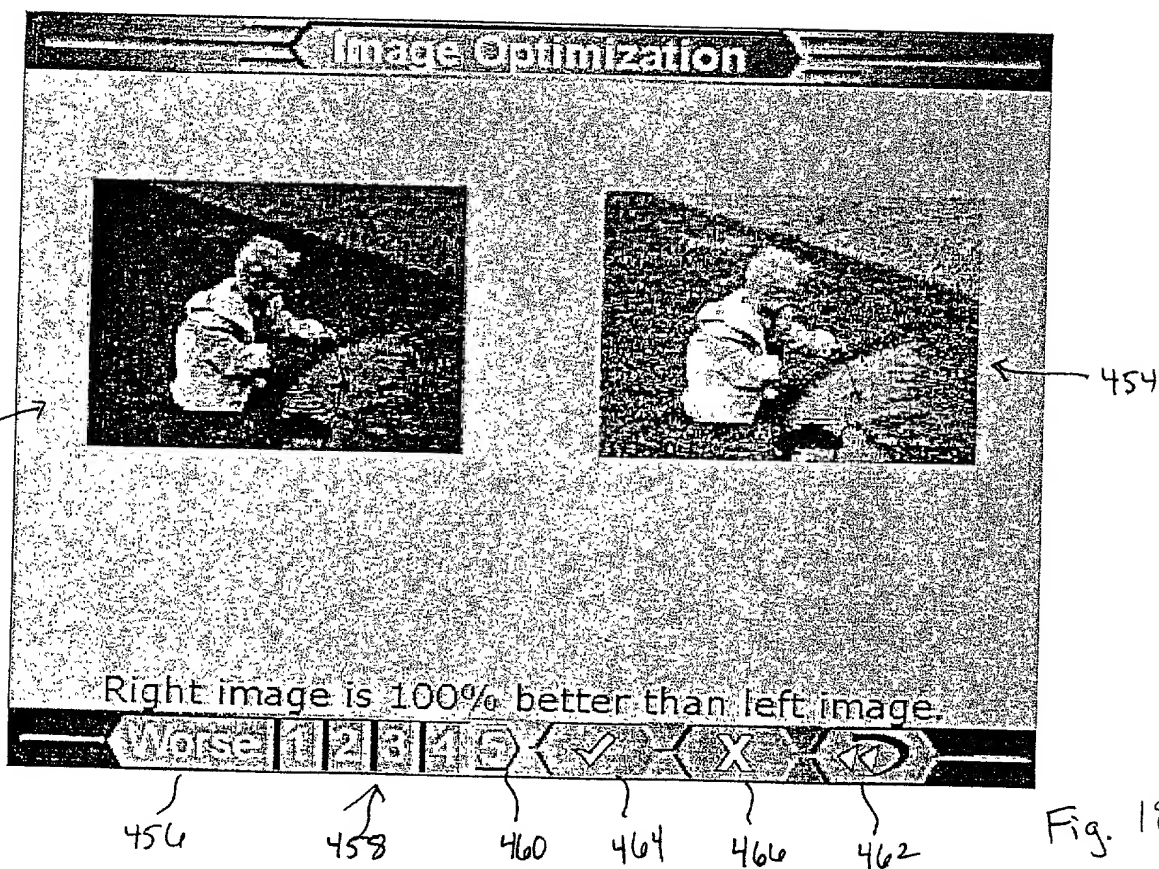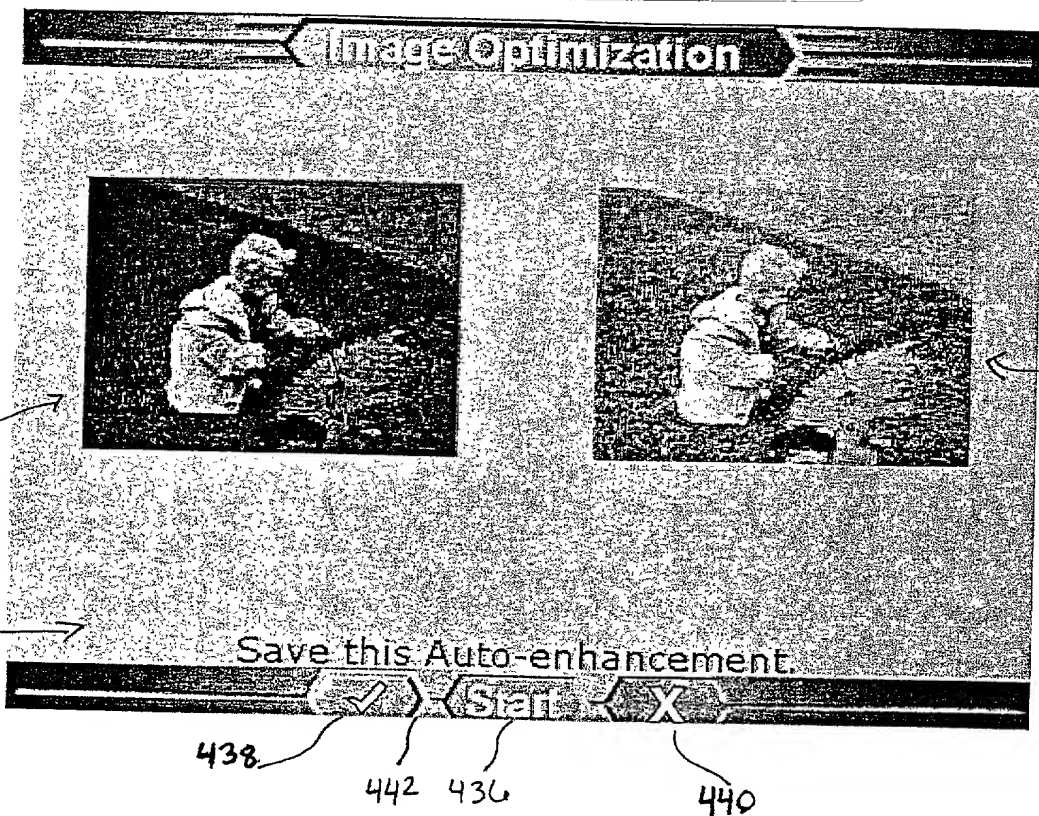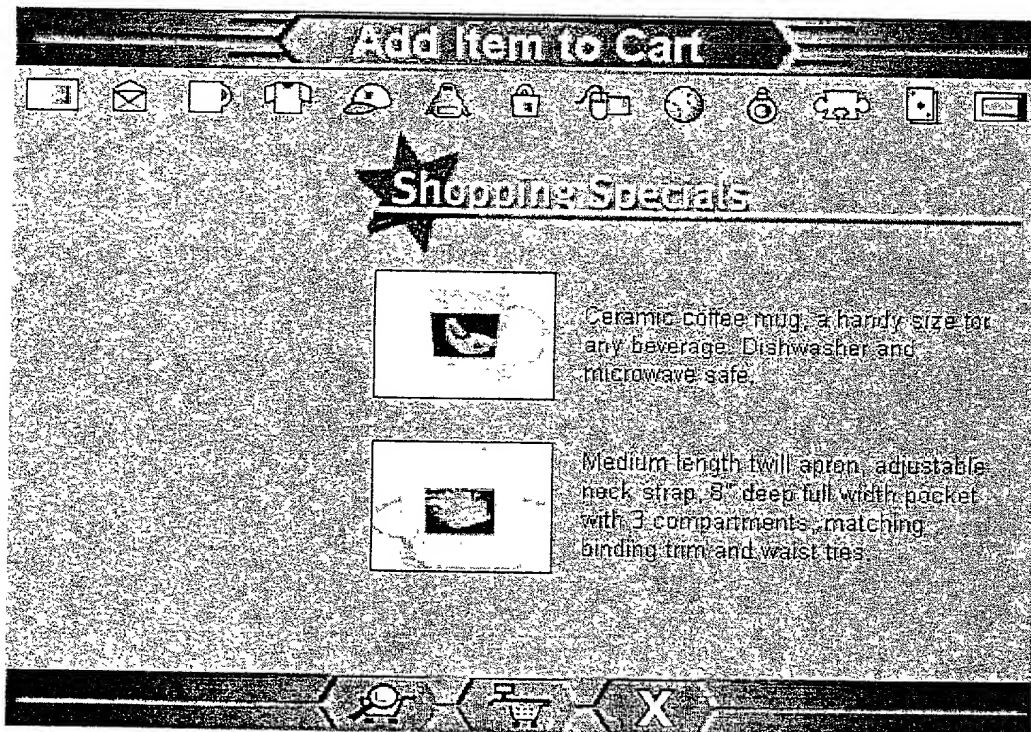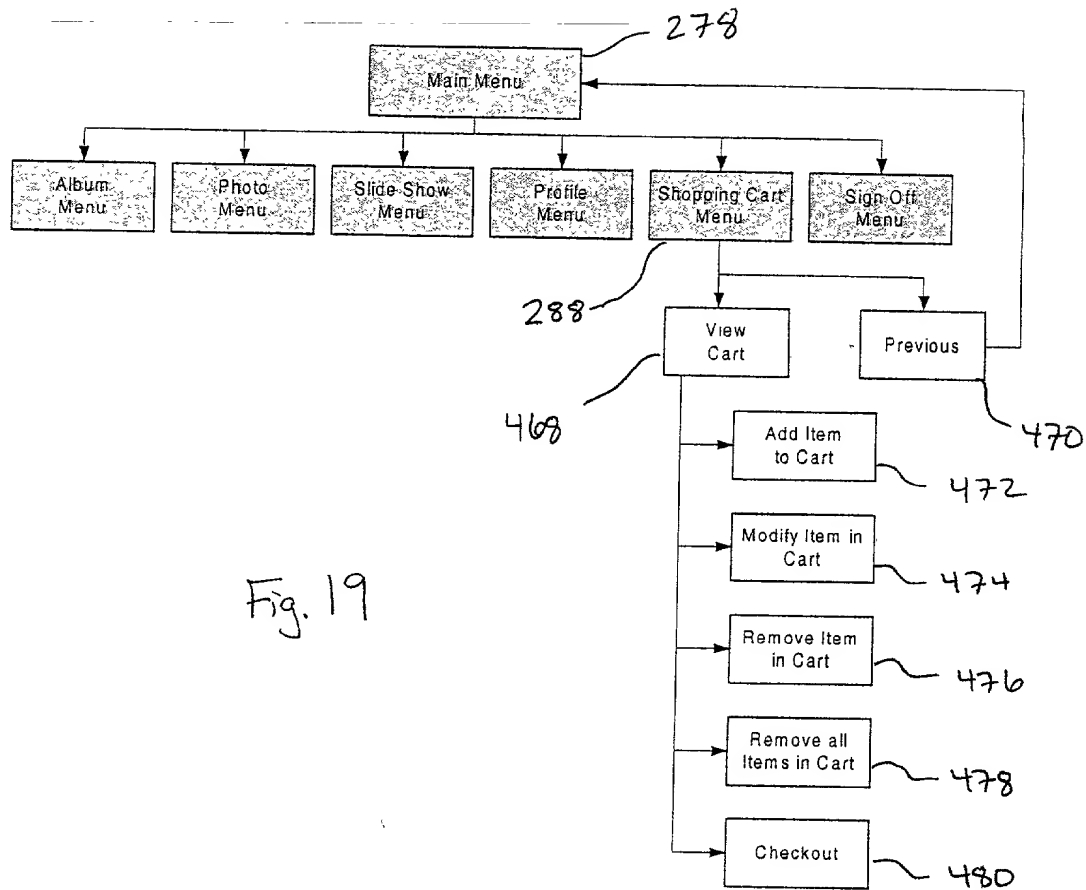

Parameter	Value	Unit
Temperature	25.0	°C
Pressure	1.0	atm
Flow rate	1.0	L/min
Concentration	0.1	mol/L
pH	7.0	
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.5	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.5	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.5	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.5	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.5	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.5	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.5	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.5	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.5	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.5	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.5	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.5	





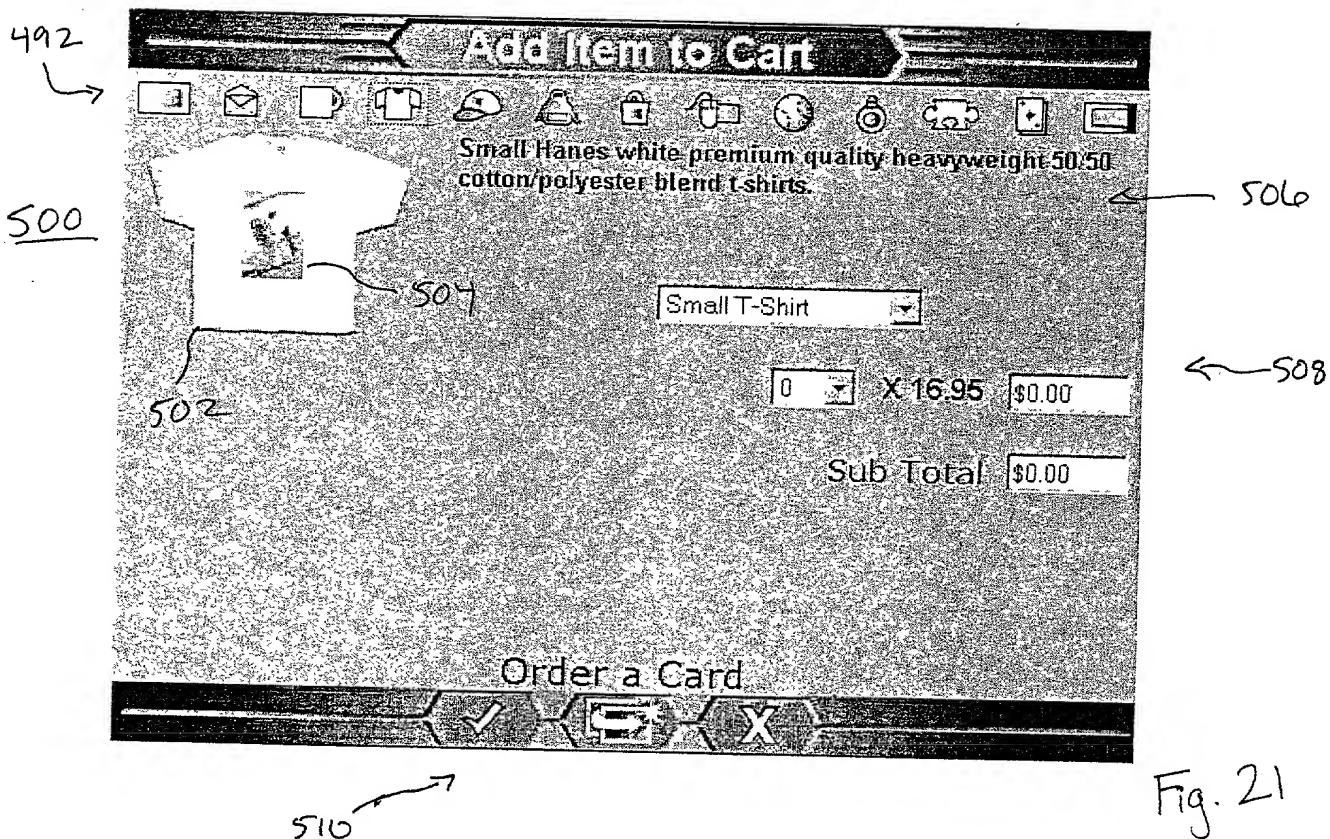


Fig. 21

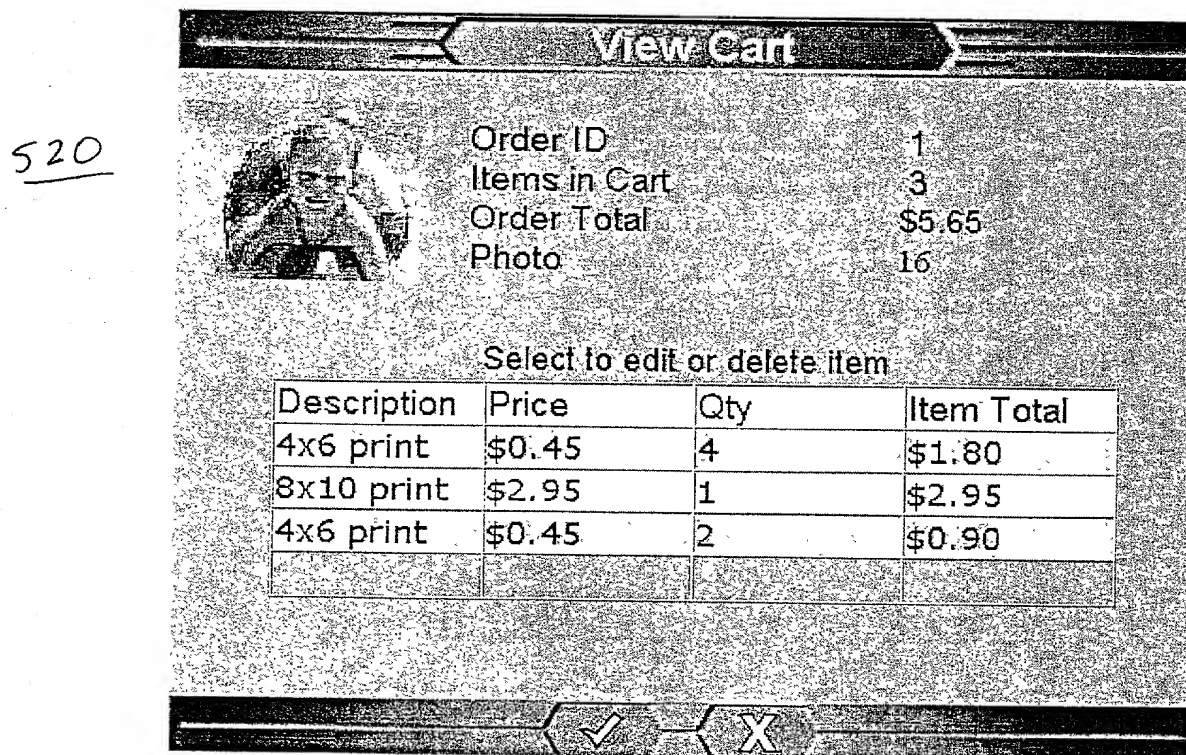


Fig. 22